

Optimal actuator location for electro-active polymer actuated endoscope [★]

Yongxin Wu ^{*} Yann Le Gorrec ^{*}

** FEMTO-ST Institute, Univ. Bourgogne Franche-Comté, ENSMM,
CNRS, 24 rue Savary, F-25000 Besançon, France.
(e-mail:yongxin.wu@femto-st.fr; yann.le.gorrec@ens2m.fr).*

Abstract: This paper deals with optimal actuator location for a medical endoscope controlled by electro-active polymer (EAP). The inner tube of the endoscope is a flexible structure that can be represented by a Timoshenko beam. Actuators are patches of EAP. There is freedom in the choice of EAP actuators location. In this paper, we first propose a port Hamiltonian model of the endoscope. In order to choose the optimal location for the EAP actuators, we consider the linear quadratic (LQ) performance as the optimal performance objective. At last, some numerical simulation results are given based on the real experimental setup parameters.

Keywords: Medical endoscope; optimal actuator location; linear quadratic optimization; port Hamiltonian system.

1. INTRODUCTION

The theoretical modeling and control of medical endoscopes have been studied since the last century (Anderson et al., 1967). In recent years, technological progresses made possible the use of continuum robots for different applications such as: laser manipulators, catheters and micro-endoscopes (Robert J. Webster and Jones, 2010). Actuated micro-endoscopes have been developed for endonasal skull base surgery in (Chikhaoui et al., 2014) with embedded actuators able to provide additional degrees of freedom to the system. In this paper, the bending of the endoscope is preformed by electro-active polymer (EAP) actuators. One of the most important EAP actuators are Ionic Polymer Composites (IPMC) whose attractive properties such as: low actuation voltage, ease of fabrication, relatively high strain and so on ... have been experimentally pointed out in (Shahinpoor and Kim, 2001).

The modeling of medical endoscopes has been considered in Chikhaoui et al. (2014) by a kinematic approach. The main body of the endoscope is a flexible structure and the IPMC actuators consist in patches of poly-electrolyte gel and metal electrodes plated by a chemical process. The modeling of such kind of system naturally leads to a complex multi physical system which is often governed by partial differential equations (PDEs). The port Hamiltonian framework is a very powerful approach for the modeling and control of mechanical, electro-mechanical and multi physical systems (Duingdam et al., 2009). Port Hamiltonian modeling is based on energy exchanges between the different components of the systems. It has been recently extended to distributed parameters systems described by partial differential equations (PDEs). The port Hamilto-

nian framework is well suited for the modeling of interconnected multiphysical systems and then particularly well adapted for the modeling of medical endoscopes. Moreover, modeling and control of flexible structures by using the port Hamiltonian framework have been widely studied in the last decade (Macchelli and Melchiorri, 2004b,a) and the port Hamiltonian modeling of IPMC soft actuators has been introduced in Nishida et al. (2011). The actuators being coated outside of the medical endoscope (shown in Fig. 1), this control problem can be regarded as the distributed control of a distributed parameter system and one has to decide the best location of actuators. This naturally leads to the optimal actuator location problem. This problem has been firstly introduced in the context of distributed parameters system in (Slemrod, 1989). The author in (Morris, 2011) proposes to minimize the linear quadratic cost function in order to choose the optimal actuators location. We can also find the other criteria to find the optimal actuators location in the review article (van de Wal and de Jager, 2001).

The organization of this paper is the following. In Section 2, we introduce the port Hamiltonian modeling of the endoscope with its distributed control. The optimal actuator location is considered by minimizing the linear quadratic cost functional in Section 3. In Section 4 is given the discretized model of the endoscope and this model is validated through several simulations. At last, we give the conclusion of this work and some remarks for future works.

2. PORT HAMILTONIAN MODELING OF ENDOSCOPE

A simplified model of a compliant endoscope used for medical examination (Chikhaoui et al., 2014) is presented in Fig 2. The inner tube is actuated by electro-active polymers (EAP) caught on the body of the endoscope. The modeling of EAP can be found in (Nishida et al., 2011). In this paper we do not represent the physical

[★] The authors gratefully acknowledge the support of the ANR-DFG (French-German) project INFIDHEM with Reference Code ANR-16-CE92-0028 and the support of the ENSMM BQR project with Reference Code BQR ENSMM N°06.2017

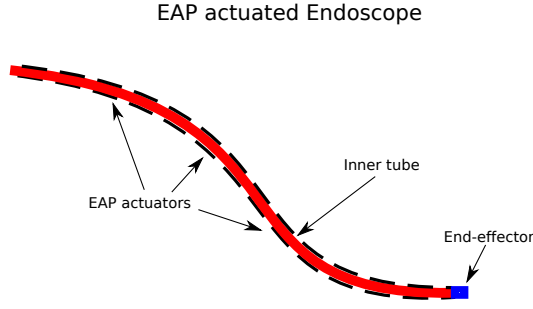


Fig. 1. EAP actuated Endoscope

model of the EAP and consider only the distributed forces and torques applied on the body of the inner tube. The compliant inner tube of the endoscope can be regarded as a flexible beam. One end of this beam is clamped while the other one is free. The actuators and the beam are interconnected through the power conjugated variables. The interconnection relation and causality are indicated also in Fig 2. The compliant inner tube is modeled as an infinite dimensional Timoshenko beam model. In the following subsections we discuss the modeling of this compliant structure and its distributed control.

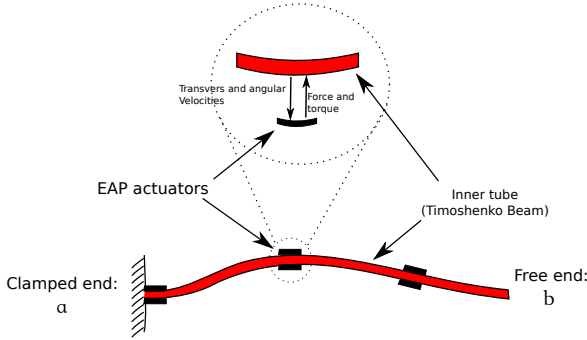


Fig. 2. Simplified EAP actuated Endoscope

2.1 Timoshenko beam

The distributed parameters port Hamiltonian formulation of Timoshenko beam has been represented in (Macchelli and Melchiorri, 2004b; Jacob and Zwart, 2012). This representation has been widely studied for the boundary control problem (Villegas et al., 2009; Ramirez et al., 2014) as well as for the distributed control problem (Macchelli, 2003) of beams. Let consider the port Hamiltonian representation of the Timoshenko beam as follows:

$$\dot{x}(t) = \underbrace{\left(P_1 \frac{\partial}{\partial z} + P_0 \right)}_{\mathcal{J}} \mathcal{L}x(t) \quad (1)$$

with the operator:

$$\mathcal{L} = \begin{bmatrix} K & 0 & 0 & 0 \\ 0 & \frac{1}{\rho} & 0 & 0 \\ 0 & 0 & EI & 0 \\ 0 & 0 & 0 & \frac{1}{I_\rho} \end{bmatrix}, \quad (2)$$

and the matrices:

$$P_1 = \begin{bmatrix} 0 & 1 & 0 & 0 \\ 1 & 0 & 0 & 0 \\ 0 & 0 & 0 & 1 \\ 0 & 0 & 1 & 0 \end{bmatrix}, P_0 = \begin{bmatrix} 0 & 0 & 0 & -1 \\ 0 & 0 & 0 & 0 \\ 0 & 0 & 0 & 0 \\ 1 & 0 & 0 & 0 \end{bmatrix}. \quad (3)$$

The state (energy) variables are the shear displacement $x_1 = \frac{\partial w}{\partial z}(z, t) - \phi(z, t)$, the transverse momentum distribution $x_2 = \rho(z) \frac{\partial w}{\partial t}(z, t)$, the angular displacement $x_3 = \frac{\partial \phi}{\partial z}(z, t)$ and the angular momentum distribution $x_4 = I_\rho \frac{\partial \phi}{\partial t}(z, t)$ for $z \in (a, b)$, $t \geq 0$, where $w(z, t)$ is the transverse displacement and $\phi(z, t)$ is the rotation angle of the beam. The coefficients ρ , I_ρ , E , I and K are the mass per unit length, the angular moment of inertia of a cross section, Young's modulus of elasticity, the moment of inertia of a cross section, and the shear modulus respectively, and the state space $X = L_2(a; b; \mathbb{R}^4)$. The energy of the beam is expressed in terms of the energy variables,

$$\begin{aligned} H &= \frac{1}{2} \int_a^b \left(Kx_1^2 + \frac{1}{\rho}x_2^2 + EIx_3^2 + \frac{1}{I_\rho}x_4^2 \right) dz \\ &= \frac{1}{2} \int_a^b x(z)^T (\mathcal{L}x)(z) dz = \frac{1}{2} \|x\|_{\mathcal{L}}^2 \end{aligned} \quad (4)$$

The medical endoscope is clamped at one end while the other end is free. The endoscope is actuated in its domain by the use of EAP patches but does not have any control at the boundary. Thus, the boundary conditions of the endoscope are $Kx_1(b, t) = EIx_3(b, t) = 0 \forall t \geq 0$ and $\frac{1}{\rho}x_2(a, t) = \frac{1}{I_\rho}x_4(a, t) = 0 \forall t \geq 0$, The domain of the operator \mathcal{J} is

$$D(\mathcal{J}) = \left\{ x \in H_1(0, 1; \mathbb{R}^n) \left| \begin{array}{l} x_2(a, t) = 0 \\ x_4(a, t) = 0 \\ x_1(b, t) = 0 \\ x_3(b, t) = 0 \end{array} \right. , \forall t \geq 0 \right\} \subset X \quad (5)$$

The operator $\mathcal{J} = P_1 \frac{\partial}{\partial z} + P_0$ defined by the matrices $P_1 = P_1^T$ and $P_0 = -P_0^T$ is a first order skew adjoint differential operator acting on the state space X with the boundary condition (5). We also consider the material of the endoscope is uniform, *i.e.* ρ , I_ρ , E , I and K are constant. Hence the operator \mathcal{L} is self-adjoint and coercive.

2.2 Distributed control of Timoshenko beam

As previously mentioned, the endoscope is controlled by the EAP actuators caught on its body. In this section, we discuss the distributed control of the inner tube body (Timoshenko beam).

Assume the EAP actuators can provide uniform torques. We place the EAP actuators on the different small intervals $I_i = [a_i, b_i]$ of the beam (on the spatial domain $[a, b]$). The torque given by each EAP can be written as $b_i(z)u_i(t)$ with $b_i(z) = 1$ if $z \in I_{b_i}$ and $b_i(z) = 0$ elsewhere.

The torque given by each EAP is $b_i(z)u_i(t)$ on the i -th on the small interval $I_i = [a_i, b_i]$ of the spatial space $[a, b]$ *i.e.* $b_i(z) = 1$ if $z \in I_{b_i}$ and $b_i(z) = 0$ elsewhere. Thus the input operator and input are:

$$\mathcal{B}(z)u(t) = \sum_i \begin{bmatrix} 0 \\ 0 \\ 0 \\ b_i(z) \end{bmatrix} u_i(t) = \begin{bmatrix} 0 \\ 0 \\ 0 \\ b(z) \end{bmatrix} u(t) \quad (6)$$

where $\mathcal{B} : \mathcal{C}^i \mapsto X$, $b(z) = [b_1(z), \dots, b_i(z), \dots]$ and $u(z) = [u_1(z), \dots, u_i(z), \dots]^T$.

Example 1. Consider that three EAP actuators are placed on the three small intervals of the beam $I_1 = [0, 0.1c]$, $I_2 = [0, 4c, 0.5c]$ and $I_3 = [0.9c, 1c]$ with $c = \frac{b-a}{10}$. The three inputs given by the three actuators are $u_1(t)$, $u_2(t)$ and $u_3(t)$. Thus the distributed control is given by

$$\mathcal{B}u = \begin{bmatrix} 0 & 0 & 0 \\ 0 & 0 & 0 \\ 0 & 0 & 0 \\ b_1(z) & b_2(z) & b_3(z) \end{bmatrix} \begin{bmatrix} u_1(t) \\ u_2(t) \\ u_3(t) \end{bmatrix} \quad (7)$$

where

$$b_i(z) \begin{cases} = 1 & \text{if } z \in I_i \\ = 0 & \text{if } z \notin I_i \end{cases} \quad i \in \{1, 2, 3\}. \quad (8)$$

The output is power conjugated to the input, *i.e.*

$$y = \mathcal{B}^* \mathcal{L}x(t) \quad (9)$$

The input-output model of the endoscope can be described by the following port Hamiltonian formulation :

$$\begin{aligned} \dot{x}(t) &= \mathcal{J}\mathcal{L}x(t) + \mathcal{B}u(t) \\ y(t) &= \mathcal{B}^* \mathcal{L}x(t) \end{aligned} \quad (10)$$

The energy balance equation can be easily computed by using the total energy of the system (4) and the system (10):

$$\frac{\partial H}{\partial t} = y^T u. \quad (11)$$

3. LINEAR QUADRATIC OPTIMAL LOCATION

In this section, we discuss the optimal actuators placement that minimizes a quadratic performance criterion. Before analyzing the optimal location problem, let recall the linear-quadratic regulator problem (Curtain and Zwart, 1995). The linear-quadratic optimal control design consists to find a control law $u(t)$ that minimizes the cost functional:

$$J_{co}(u, x_0) = \int_0^\infty (\langle x(t), Qx(t) \rangle + \langle u(t), Ru(t) \rangle) dt \quad (12)$$

$x(t) \in X$ is the state variable defined in (1). The state and control weighting operators $Q : X \mapsto X$ and $R : \mathcal{U} \mapsto \mathcal{U}$ are bounded, symmetric and positive definite.

Definition 2. The system (10) with cost functional (12) is optimizable if for every $x_0 \in X$, there exists $u \in L_2([0, \infty); \mathcal{U})$ such that the cost is finite.

Definition 3. The pair $(Q^{1/2}, \mathcal{J}\mathcal{L})$ is detectable if there exists $F : \mathcal{Y} \mapsto X$ such that $\mathcal{J}\mathcal{L} - \mathcal{F}\mathcal{C}$ generates an exponentially stable semigroup.

Theorem 4. (Curtain and Zwart, 1995) If the system (10) with cost functional (12) is optimizable and detectable, then the cost function has a minimum for every $x_0 \in X$. Furthermore, there exists a self-adjoint non-negative operator $P : X \mapsto X$ such that

$$\min_{u \in L_2([0, \infty); \mathcal{U})} J_{co}(u, x_0) = \langle x_0, Px_0 \rangle \quad (13)$$

The operator P is the non-negative unique solution of the Riccati equation:

$$((\mathcal{J}\mathcal{L})^*P + P\mathcal{J}\mathcal{L} - P\mathcal{B}^T R \mathcal{B}P + Q)x = 0 \quad (14)$$

with $x \in D(\mathcal{L})$. Defining $K = R^{-1}\mathcal{B}^*P$, the optimal control is $u = -Kx(t)$ and $\mathcal{J}\mathcal{L} - \mathcal{B}K$ generates an exponentially stable semigroup.

Definition 5. The pair $(\mathcal{J}\mathcal{L}, \mathcal{B})$ is stabilizable if there exists $K : \mathcal{U} \mapsto X$ such that $\mathcal{J}\mathcal{L} - \mathcal{B}K$ generates an exponentially stable semigroup.

Let us now consider m actuators of which the location can be varied over the compact set Ω . We parametrize their location by r . The input operator is denoted as $\mathcal{B}(r)$ and depends on the parameter r . This parameter r is a vector of length m with components in Ω so r is varied on the space denoted by Ω^m . Hence for each r we have an optimal control problem (12) which we denote by $J_{co}^r(u, x_0)$ corresponding to the optimal cost $\langle x_0, P(r)x_0 \rangle$.

Normally, the initial condition x_0 is not fixed. In this paper, we consider that the optimal location minimizes the cost function associated to the worst choice of the initial condition (Curtain and Zwart, 1995, Lemma A.3.70), *i.e.* we choose r in order to minimize

$$\max_{\substack{x_0 \in X \\ \|x_0\| = 1}} \min_{u \in L_2([0, \infty); \mathcal{U})} J_{co}^r(u, x_0) = \max_{\substack{x_0 \in X \\ \|x_0\| = 1}} \langle x_0, Px_0 \rangle = \|P(r)\|. \quad (15)$$

We denote the performance at location r , $\mu(r) = \|P(r)\|$ and the optimal performance

$$\hat{\mu} = \inf_{r \in \Omega^m} \|P(r)\|. \quad (16)$$

Theorem 6. (Morris, 2011) Let $\mathcal{B}(r) : \mathcal{U} \mapsto X$, $r \in \Omega^m$, be a family of input operators such that for any $r_0 \in \Omega^m$

$$\lim_{r \rightarrow r_0} \|\mathcal{B}(r) - \mathcal{B}(r_0)\| = 0. \quad (17)$$

Assume that $(\mathcal{J}\mathcal{L}, \mathcal{B}(r))$ are all exponentially stabilizable and that $(Q^{1/2}, \mathcal{J}\mathcal{L})$ is detectable where $Q^{1/2} : X \mapsto \mathcal{Y}$ is compact. If \mathcal{U} and \mathcal{Y} are finite dimensional, then there exists an optimal actuator location \hat{r} such that

$$\|\hat{r}\|_1 = \inf_{r \in \Omega^m} \|r\|_1 = \hat{\mu} \quad (18)$$

Theorem 6 shows that we can find the optimal actuators location if the input operators $\mathcal{B}(r)$ and the operator $Q^{1/2}$ are compact. Riccati equations have unique non-negative solutions, then the optimal location with performance $\hat{\mu} = \inf_{r \in \Omega^m} \|P(r)\|$ exists. This result is proven following Theorem 3.1 of (Curtain and Sasane, 2001).

4. COMPUTATION OF THE OPTIMAL LOCATION AND SIMULATION RESULTS

In this section, we discuss the optimal location of EAP actuators for the control of the beam position.

We first focus on the one actuator case. We then discuss two different situations. First, we consider the optimal actuator location when the power conjugate output of the port Hamiltonian system is measured. Second, we consider the optimal actuator location when the output signal is measured at the middle of the beam.

The system (10) can be represented as:

$$\dot{x}(t) = \mathcal{J}\mathcal{L}x(t) + \mathcal{B}(r)(z)u(t) \quad (19)$$

The input operator $\mathcal{B}(r)$ depends on the actuator location r . We denote Δ the length of the actuator. Thus the input operator can be written as:

$$\mathcal{B}(r) = \begin{bmatrix} 0 \\ 0 \\ 0 \\ b_r(z) \end{bmatrix} \quad \text{with } b_r(z) = \begin{cases} 1, & |r - z| < \frac{1}{\Delta} \\ 0, & |r - z| > \frac{1}{\Delta} \end{cases}. \quad (20)$$

The power conjugated output is

$$y(t) = \mathcal{B}^*(r)\mathcal{L}x(t), \quad (21)$$

which also depends on the actuator location r . Consider the state weighting operator $Q = \mathcal{L}\mathcal{B}(r)\mathcal{B}^*(r)\mathcal{L}$ and the input weighting operator $R = I$, the cost functional (12) becomes:

$$J_{co}(u, x_0) = \int_0^\infty (\langle y(t), y(t) \rangle + \langle u(t), u(t) \rangle) dt. \quad (22)$$

The optimal objective is to minimize the norm of the response over time. The Riccati equation associated with this optimal problem is

$$((\mathcal{J}\mathcal{L})^*P + P\mathcal{J}\mathcal{L} - P\mathcal{B}(r)\mathcal{B}^*(r)P + \mathcal{L}\mathcal{B}(r)\mathcal{B}^*(r)\mathcal{L})x = 0 \quad (23)$$

with $x \in D(\mathcal{L})$. Since the operator Riccati equation (23) cannot be solved in practice, we need an approximation of the system (19) to compute the control law. We discuss the discretization of the system (10) in the next paragraph.

We use the mixed-finite element discretization method proposed in (Golo et al., 2004). The idea of this method is to approximate flows and efforts with different functions in order to preserve the physical meaning of each variable and the geometric structure of the system. In the case of the Timoshenko beam, defined on a one-dimensional spatial domain, the effort variables (torque) correspond to some zero (differential) forms (functions) and the flow variables (angular velocities) correspond to some one (differential) forms respectively. This spatial discretization method has been applied to different physical models, the reader can read (Hamroun et al., 2009; Baaiu et al., 2009) for more details and (Macchelli et al., 2009) for a specific application to the Timoshenko beam. The explicit finite dimensional port Hamiltonian approximation of the Timoshenko beam is given by:

$$\dot{x}_d = J_d \frac{\partial H_d}{\partial x_d} + B_d(r)u \quad (24)$$

where $J_d = -J_d^T \in \mathbb{R}^{4N}$ with N the number of infinitesimal subsections used for the discretization, $H_d = \frac{1}{2}x_d^T L_d x_d$ is the Hamiltonian function with L_d the approximation matrix of operator \mathcal{L} . The following matrices present the discretized structure operator of the infinite dimensional model :

$$J_d = \underbrace{\begin{bmatrix} 0 & M & 0 & 0 \\ M^T & 0 & 0 & 0 \\ 0 & 0 & 0 & M \\ 0 & 0 & M^T & 0 \end{bmatrix}}_{\bar{P}_1} + \underbrace{\begin{bmatrix} 0 & 0 & 0 & -\Phi \\ 0 & 0 & 0 & 0 \\ 0 & 0 & 0 & 0 \\ \Phi^T & 0 & 0 & 0 \end{bmatrix}}_{\bar{P}_2} \quad (25)$$

where the sub-matrices are:

$$M = \begin{bmatrix} -1 & 1 & 0 & \cdots & 0 \\ 0 & -1 & 1 & \ddots & \vdots \\ \vdots & \ddots & \ddots & \ddots & 1 \\ 0 & \cdots & 0 & 0 & -1 \end{bmatrix} \quad \text{with } M \in \mathbb{R}^{N \times N} \quad (26)$$

$$\Phi = \text{diag}(\beta, \dots, \beta) \quad \text{with } \Phi \in \mathbb{R}^{N \times N} \quad (27)$$

where β is the size of the infinitesimal section. The matrix $B_d(r)$ is the approximation of the input operator $\mathcal{B}(r)$:

$$B_d(r) = \begin{bmatrix} 0 \\ 0 \\ 0 \\ b_r \end{bmatrix} \in \mathbb{R}^{4N} \quad (28)$$

where the vector $b_r \in \mathbb{R}^N$ depends on the actuator location r . By using approximation (24) of system (19), we can get an approximate solution P_d from the resolution of the following finite dimensional Riccati equation:

$$(J_d L_d)^T P_d + P_d J_d L_d - P_d B_d(r) B_d^T(r) P_d + L_d B_d(r) B_d^T(r) L_d = 0. \quad (29)$$

We consider now the numerical simulation of this optimal actuator location. The parameters used for this simulation are given in Tab. 1. These are the real parameters of the experimental setup built in department AS2M of Institute FEMTO-ST (shown in Fig. 3).

Parameters of beam and actuator	Value (unit)
Length L	30 cm
Width b	2 cm
Thickness h	2 mm
Young's modulus E	0.2 GPa
Mass density ρ	920 kg/m ²
Actuator length Δ	3 cm

Table 1. Parameters of the beam

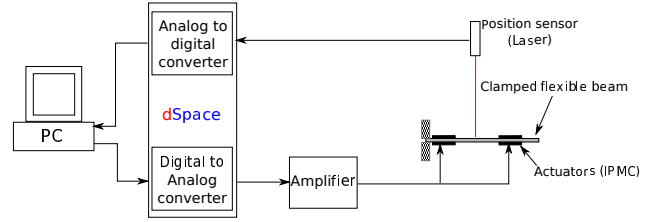


Fig. 3. Clamped flexible beam experimental setup

We illustrate the optimal actuator location for system (19) with the LQ cost function (22). The actuator is ten times shorter than the beam *i.e.* $\Delta = \frac{b-a}{10}$. The optimal actuator location is computed by using the approximation (24) with different numbers of infinitesimal subsection (N). We vary N from 10 to 200. The optimal actuator location is illustrated in Fig 4. In this simulation result, we see that in the power conjugated input-output case, *i.e.* $Y = \mathcal{B}^*(r)\mathcal{L}x$, the optimal actuator location is at the clamped side of the beam.

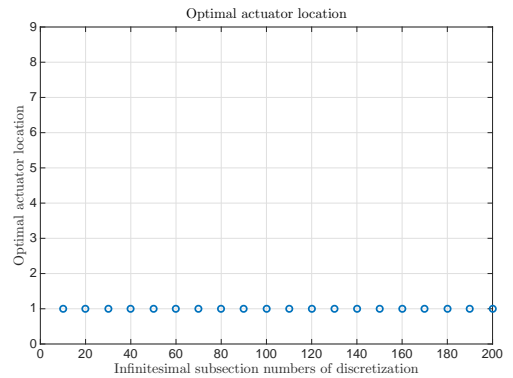


Fig. 4. Optimal location

In Fig. 5, are shown the LQ-performance $\|P\|$ for the different actuator locations. This variation of the LQ norm $\|P(r)\|$ has been computed for $N = 60$. The actuator location is evaluated considering each finite element of discretization from the clamped side to the free side of the beam. The actuator location which minimizes the LQ-norm $\|P(r)\|$ is at the clamped side.

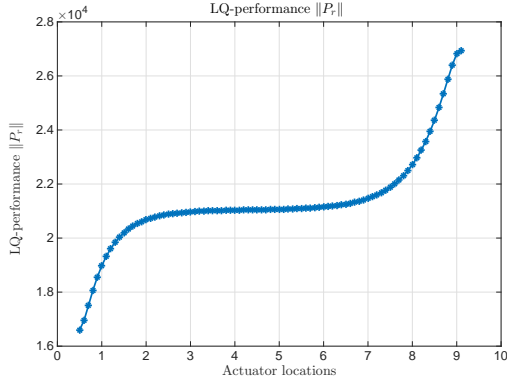


Fig. 5. Variation of LQ performance $\|P\|$ with respect to actuator location

We consider now the second case of study where the measurement is the displacement at the middle of the beam. In this situation, the output of the system is

$$y_2(t) = \mathcal{B}^* \mathcal{L}x(t), \quad (30)$$

with

$$\mathcal{B} = \begin{bmatrix} 0 \\ 0 \\ 0 \\ b(z) \end{bmatrix} \quad \text{with } b(z) = \begin{cases} 1, & z \in I \\ 0, & z \notin I \end{cases} \quad (31)$$

where I is a small interval $I = [0.4c, 0.5c]$, $c = \frac{b-a}{10}$.

The cost functional of the LQ problem can be written as follows:

$$J_{co}(u, x_0) = \int_0^\infty (\langle y_2(t), y_2(t) \rangle + \langle u(t), u(t) \rangle) dt. \quad (32)$$

with state weighting operator $Q = \mathcal{L}\mathcal{B}\mathcal{B}^*\mathcal{L}$. Then the objective becomes to minimize the norm of the response within the fixed interval $I = [0.4c, 0.5c]$ over time.

We illustrate the optimal actuator location of the above LQ optimal problem by Fig. 6. We can see the optimal actuator location is not the same as the one shown in Fig. 4 because of the change of the LQ cost functional. The optimal actuator location we find is collocated to the measurement. In Fig. 7, we show the LQ-performances $\|P\|$ for the different actuator locations. The variation of the LQ norm $\|P(r)\|$ has been computed for $N = 60$. This simulation result shows that we have to place the actuator in the interval $I = [0.4c, 0.5c]$ in order to minimize the norm of the response over time in the same interval. This results in collocated input and output. After several simulations (which are not shown in this paper), the optimal actuator locations are always collocated to the output measurements.

Now we consider two actuators. We suppose that the measurements are the displacement at the intervals $I = [0.2c, 0.3c]$ and $I = [0.5c, 0.6c]$. Fig. 8 shows that the

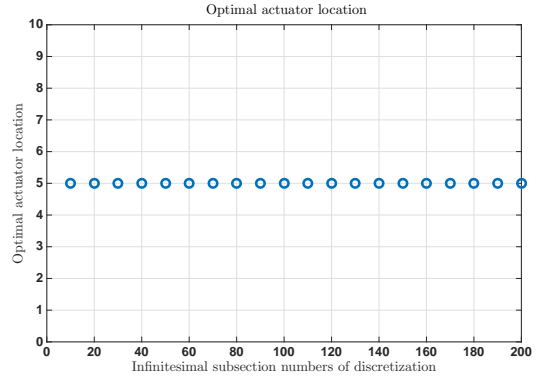


Fig. 6. Optimal location

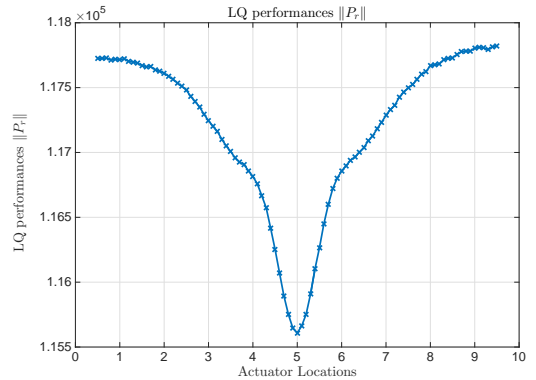


Fig. 7. Variation of LQ performance $\|P\|$ with respect to actuator location

optimal actuator locations are also around these two intervals. The variation of the LQ norm $\|P(r)\|$ has been computed for $N = 100$. In this figure, we can see that the anti-diagonal elements situated from the bottom left to the top right have no meaning as they correspond to superimposed actuators. They do not have real physical meaning in practical application. This simulation shows similar result as in the one actuator case.

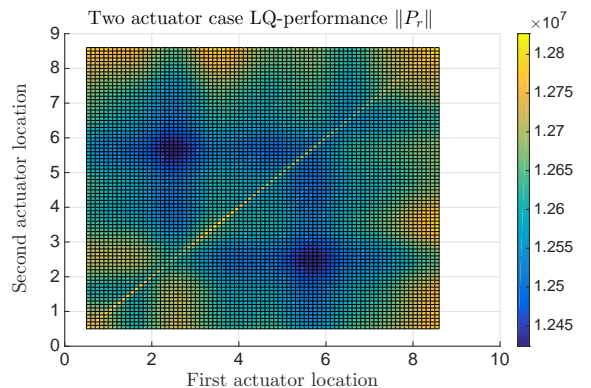


Fig. 8. Actuators locations

5. CONCLUSION AND FUTURE WORK

In this paper, the port Hamiltonian framework has been used for the modeling and the discretization of a class of bio-medical endoscopes. These medical endoscopes are controlled by the use of distributed torques provided

by EAP actuators. We have formulated the endoscope and its distributed control as an abstract system by the port Hamiltonian approach. Then we have considered a LQ optimal actuator location problem for this system. This optimal problem consists in the minimization of the LQ cost functions which are related to the actuator locations. This method has been illustrated by numerical simulations. The parameters of a real experimental setup have been used in this simulation.

The ongoing work is the implementation of this method on the experimental benchmark in order to compare the experimental results with the numerical ones. Since the EAP can also be used as deformation sensors, we will consider both optimal sensor/actuator locations in a future work.

REFERENCES

- Anderson, V., Horn, R., and of Mechanical Engineers, A.S. (1967). *Tensor Arm Manipulator Design*. American Society of Mechanical Engineers. Papers. American Society of Mechanical Engineers.
- Baaiu, A., Couenne, F., Gorrec, Y.L., Lefèvre, L., and Tayakout, M. (2009). Structure-preserving infinite dimensional model reduction application to adsorption processes. *Journal of Process Control*, 19(3), 394–404.
- Chikhaoui, M.T., Rabenorosoa, K., and Andreff, N. (2014). *Kinematic Modeling of an EAP Actuated Continuum Robot for Active Micro-endoscopy*, 457–465. Springer International Publishing, Cham.
- Curtain, R.F. and Sasane, A.J. (2001). Compactness and nuclearity of the hankel operator and internal stability of infinite-dimensional state linear systems. *International Journal of Control*, 74(12), 1260–1270. doi:10.1080/00207170110061059.
- Curtain, R. and Zwart, H. (1995). *An introduction to Infinite-Dimensional Linear System Theory*. Springer-Verlag, i edition. ISBN 0-387-94475-3.
- Duindam, V., Macchelli, A., Stramigioli, S., and Bruyninckx, H.e. (2009). *Modeling and Control of Complex Physical Systems - The Port-Hamiltonian Approach*. Springer. ISBN 978-3-642-03195-3.
- Golo, G., Talasila, V., van der Schaft, A., and Maschke, B. (2004). Hamiltonian Discretization of Boundary Control Systems. *Automatica*, 40, 757–771.
- Hamroun, H., Lefèvre, L., and Mendes, E. (2009). A port-controlled Hamiltonian approach to geometric reduction of distributed parameters systems - application to the shallow water equations. *International Journal of Numerical Methods in Engineering*.
- Jacob, B. and Zwart, H.J. (2012). *Linear Port-Hamiltonian Systems on Infinite-dimensional Spaces*, volume 223 of *Operator Theory: Advances and Applications*. Springer Basel.
- Macchelli, A. and Melchiorri, C. (2004a). Control by Interconnection and Energy Shaping of the Timoshenko Beam. *Journal of Mathematical and Computer Modelling of Dynamical Systems*, 10, 231–251.
- Macchelli, A. and Melchiorri, C. (2004b). Modeling and control of the Timoshenko beam. the Distributed Port Hamiltonian approach. *SIAM Journal On Control and Optimization*, 43(2), 743–767.
- Macchelli, A., Melchiorri, C., and Stramigioli, S. (2009). Port-based modelling and simulation of mechanical systems with rigid and flexible links. *IEEE Trans. on Robotics*, 25(5), 1016–1029.
- Macchelli, A. (2003). *Port Hamiltonian Systems - A unified approach for modeling and control finite and infinite dimensional physical systems*. Ph.D. thesis, University of Bologna, Bologna, Italy.
- Morris, K. (2011). Linear-quadratic optimal actuator location. *IEEE Transactions on Automatic Control*, 56(1), 113–124.
- Nishida, G., Takagi, K., Maschke, B., and Osada, T. (2011). Multi-scale distributed parameter modeling of ionic polymer-metal composite soft actuator. *Control Engineering Practice*, 19(4), 321 – 334. doi:DOI: 10.1016/j.conengprac.2010.10.005.
- Ramrez, H., Gorrec, Y.L., Macchelli, A., and Zwart, H. (2014). Exponential stabilization of boundary controlled port-hamiltonian systems with dynamic feedback. *IEEE Transactions on Automatic Control*, 59(10), 2849–2855.
- Robert J. Webster, I. and Jones, B.A. (2010). Design and kinematic modeling of constant curvature continuum robots: A review. *The International Journal of Robotics Research*, 29(13), 1661–1683.
- Shahinpoor, M. and Kim, K.J. (2001). Ionic polymer-metal composites: I. fundamentals. *Smart Materials and Structures*, 10(4), 819.
- Slemrod, M. (1989). Sensors and controls in the analysis of distributed systems (a. el jai and a. j. pritchard). *SIAM Review*, 31(4), 710–710.
- van de Wal, M. and de Jager, B. (2001). A review of methods for input/output selection. *Automatica*, 37(4), 487 – 510.
- Villegas, J., Zwart, H., Le Gorrec, Y., and Maschke, B. (2009). Stability and stabilization of a class of boundary control systems. *IEEE Transaction on Automatic Control*, 54(1), 142–147. doi:10.1109/TAC.2008.2007176.